

Plasma/Serum cfc-DNA Advanced Purification Kit
Product # 68000
Product Insert
Introduction

Cell-Free Circulating DNA (cfc-DNA) resulting from apoptosis, and circulating tumour DNA (ct-DNA) released due to the apoptosis and/or the necrosis of tumour cells, has been found in blood plasma/serum and other bodily fluids. Analyzing cfc-DNA and/or ct-DNA from plasma has now become an important tool in the oncology field for the analysis of the molecular changes taking place during the development or the progress of cancerous cells. Cfc-DNA/ct-DNA has the potential to provide biomarkers for certain cancers and disease states as well as fetal DNA in maternal blood. Corresponding to the size of the chromosome (core histones + linker), cfc-DNA is mostly found in plasma around the size of 167 bp, whereas ct-DNA is usually found around the size of 145 bp. Ct-DNA, in the plasma acquired from cancer patients, accounts for ~10% of the total cfc-DNA which is normally present in very low concentrations. Most current plasma/serum cfc-DNA/ct-DNA purification methods isolate total DNA from plasma or serum with high genomic DNA (gDNA) contamination that usually results due to the lysis of white blood cells (WBCs) during blood collection, plasma/serum preparation and/or storage/preservation/transport of blood samples. This gDNA contamination will mask cfc-DNA/ct-DNA normally present in low concentrations, leading to unreliable results. In addition, cell-free fetal DNA has been widely used as a non-invasive method for prenatal diagnosis including early identification of fetal sex, genetic studies for families at high risk for inherited genetic disorders, screening for Rhesus factor, screening for aneuploidy and identification of preeclampsia.

Norgen's Plasma/Serum cfc-DNA Advanced Purification Kit provides fast, reliable and simple procedures for isolating the highest quality and quantity of cell-free circulating DNA (cfc-DNA) from various amounts of plasma/serum ranging from 1 mL up to 6 mL with minimal genomic DNA (gDNA) contamination. Isolation is based on using Norgen's proprietary resin separation matrix. The kit is designed to isolate all sizes of cfc-DNA and ct-DNA from either fresh, preserved or frozen plasma/serum samples. Moreover, this kit allows the user to elute the purified cfc-DNA into a flexible elution volume ranging from 25 µL to 50 µL. The purified plasma/serum cfc-DNA is eluted in an Elution Buffer that is compatible with all downstream applications including PCR, qPCR, methylation-sensitive PCR and Southern Blot analysis, microarrays and NGS.

Kit Components:

Component	Product # 68000 (50 preps)
Binding Buffer A	20 mL
Proteinase K	6.5 mL
Slurry E	12.5 mL
Lysis Buffer A	130 mL
Wash Solution A	38 mL
Elution Buffer C	2 x 8 mL
Elution Buffer F	1 x 15 mL 1 x 6 mL
Micro Spin Columns	50
Mini Filter Spin Column	50
Collection Tubes	100
Elution tubes (1.7 mL)	100
Product Insert	1

The kit is compatible with the isolation of cfc-DNA from fresh, preserved or frozen serum/plasma prepared from blood collected on either Norgen's cf-DNA/cf-RNA Preservative Tubes (Cat. 63950, 63960), Cell-Free DNA BCT® (Streck), Heparin, EDTA or Citrate.

*** Please check Appendix A for Average Plasma/Serum Yields and Common DNA Quantification Methods.**

Customer-Supplied Reagents and Equipment for Manual Isolation

- Benchtop microcentrifuge
- Swinging bucket centrifuge
- Micropipettors
- 15 mL tubes
- 96 – 100% ethanol

Storage Conditions and Product Stability

All solutions should be kept tightly sealed and stored at room temperature. This kit is stable for 2 years after the date of shipment. The kit contains a ready-to-use Proteinase K, which is dissolved in a specially prepared storage buffer. The buffered Proteinase K is stable for up to 2 years after the date of shipment when stored at room temperature.

Quality Control

In accordance with Norgen's Quality Management System, each lot of Norgen's Plasma/Serum cfc-DNA Advanced Purification Kit is tested against predetermined specifications to ensure consistent product quality.

Product Use Limitations

Norgen's Plasma/Serum cfc-DNA Advanced Purification Kit is designed for research purposes only. It is not intended for diagnostic use.

Product Warranty and Satisfaction Guarantee

NORGEN BIOTEK CORPORATION guarantees the performance of all products in the manner described in our product manual. The customer must determine the suitability of the product for its particular use.

Safety Information

Ensure that a suitable lab coat, disposable gloves and protective goggles are worn when working with chemicals. For more information, please consult the appropriate Material Safety Data Sheets (MSDSs). These are available as PDF files online at www.norgenbiotek.com.

Lysis Buffer A contains guanidine thiocyanate, and should be handled with care. Guanidine thiocyanate forms highly reactive compounds when combined with bleach, thus care must be taken to properly dispose of any of this solution.

Plasma or serum of all human and animal subjects is considered potentially infectious. All necessary precautions recommended by the appropriate authorities in the country of use should be taken when working with plasma or serum.

CAUTION: DO NOT add bleach or acidic solutions directly to the sample-preparation waste.

Important Notes

- All centrifugation steps are performed at room temperature.
- Ensure that centrifuge tubes used are capable of withstanding the centrifugal forces required.
- Most standard benchtop microcentrifuges will accommodate Norgen's Micro and Mini Filter Spin Columns.
- Centrifuging Norgen's spin columns at a speed lower than recommended in the procedure will not affect DNA yield. However, centrifugation at a lower speed may require longer time for the solutions to pass through the spin column
- Clean, disposable gloves should be worn at all times when handling reagents, samples, pipettes, disposable tubes, etc. It is recommended that gloves are changed frequently to avoid contamination.
- Ensure that all solutions are at room temperature prior to use, and that no precipitates have formed. If necessary, warm the solutions and mix well until the solutions become clear again.
- Prepare a working concentration of the **Wash Solution A** by adding **90 mL of 96 - 100% ethanol** (provided by the user) to the supplied bottle containing the **38 mL concentrated Wash Solution A**.

- This will give a final volume of 128 mL. The label on the bottle has a box that may be checked to indicate that the ethanol has been added
- Ensure that samples have not undergone more than one freeze-thaw cycle, as this may lead to DNA degradation.
 - Always **vortex** the **Proteinase K** before use.
 - It is highly recommended to warm **Lysis Buffer A** at 60°C for 20 minutes and mix well until the solutions become clear again if precipitates (crystals) are present.
 - **The kit is compatible with the isolation of cfc-DNA from fresh, preserved or frozen serum/plasma prepared from blood collected on either Norgen's cf-DNA/cf-RNA Preservative Tubes (Cat. 63950, 63960), Cell-Free DNA BCT® (Streck), Heparin, EDTA or Citrate.**
 - **If any of the solutions do not go through the Spin Columns within the specified centrifugation time, spin for an additional 1-2 minutes at maximum speed until the solution completely passes through the column.**
 - **Frozen plasma (from Blood collected on Heparin, EDTA or Citrate Tubes) or serum samples should be centrifuged for 2 minutes at 400 x g (~2,000 RPM) before processing. Only clear supernatant should be processed, as column clogging may be encountered if frozen samples are directly processed.**
 - **VERY IMPORTANT! Frozen plasma recovered from Norgen's cf-DNA/cf-RNA Preservative Tubes (Cat. 63950, 63960) may contain some precipitates upon thawing. DO NOT discard any precipitates before cfc-DNA Isolation. Briefly vortex the plasma and proceed immediately for cfc-DNA Isolation. Discarding any precipitates may significantly lower cfc-DNA yield.**

CFC-DNA Isolation from 0.5 mL up to 6 mL plasma/Serum

Important Notes:

- This procedure as written is for processing 1 mL Plasma/Serum samples. To process a different Plasma/Serum volume higher than 1 mL, please check Table 1 for the appropriate volumes of Binding Buffer A, Elution Buffer C and Proteinase K.
 - To process a different Plasma/Serum volume lower than 1 mL, please bring up the volume of your sample up to 1 mL using 1X PBS (pH 7.4) then follow the procedure outline below.
 - Please refer to the notes in the Important Notes section for the pre-treatment of frozen plasma/serum samples
1. Place 1 mL of plasma/serum sample in a 15 mL tube (provided by the user) followed by the addition of 50 µL **Binding Buffer A**. Mix well by vortexing for 20 seconds. Incubate for 5 minutes at room temperature
 2. After incubation, centrifuge for **1 minute at 50 x g (~500 RPM)**. Discard completely the supernatant.
 3. Add 34 µL **Elution Buffer C** to the pellet resulting from **Step 2**. Mix well by vortexing for 30 seconds. **(Note: The pellet resulting from Step 2 must be completely resuspended in Elution Buffer C)**
 4. Add 17 µL of **Proteinase K** to the resuspended pellet. Mix well by vortexing for 10 seconds then incubate at **room temperature for 30 minutes** with shaking slowly end-over-end.
 5. After incubation, add 200 µL **Slurry E** followed by the addition 1.5 mL of **Lysis Buffer A**, and mix well by vortexing for 10 seconds. **(Note: Slurry E contains resin and must be mixed well before every pipeting)**. Incubate for 2 minutes at room temperature.
 6. After incubation, add 2 mL **96-100% Ethanol** and mix well by vortexing for 10 seconds.
 7. Incubate for 2 minutes at room temperature then mix well by vortexing for 10 seconds.
 8. Transfer 700 µL of the mixture from **Step 7** into a Mini Spin column assembled with one of the provided collection tubes. Centrifuge for **30 seconds at 13,000 x g (~14,000 RPM)**. Discard the flowthrough and reassemble the spin column with its collection tube.
 9. Repeat **Step 8** until the entire mixture from **Step 7** is transferred into the Mini Filter Spin column.
 10. Apply 600 µL of **Wash Solution A** to the column and centrifuge for **30 seconds at 13,000 x g (~14,000 RPM)**. Discard the flowthrough and reassemble the spin column with its collection tube.

11. Repeat **Step 10** one more time for a total of two washes.
12. Spin the column, empty, for **2 minutes at 13,000 x g (~14,000 RPM)**. Discard the collection tube.
13. Transfer the spin column to a fresh 1.7 mL Elution tube. Apply 250 µL of **Elution Buffer F** to the column and let stand at room temperature for 2 minutes. Centrifuge for **1 minute at 400 x g (~2,000 RPM)**, followed by **2 minutes at 5,800 x g (~8,000 RPM)**.
14. Add 500 µL of **Lysis Buffer A** to the eluted DNA, and mix well by vortexing for 10 seconds
15. Add 750 µL **96-100% Ethanol** and mix well by vortexing for 10 seconds.
16. Transfer 500 µL of the mixture into a Micro Spin column assembled with one of the provided collection tubes. Centrifuge for **1 minute at 3,300 x g (~6,000 RPM)**. Discard the flowthrough and reassemble the spin column with its collection tube.
17. Repeat **Step 16** one more time to transfer the remaining mixture from **Step 15**.
18. Apply 600 µL of **Wash Solution A** to the column and centrifuge for **1 minute at 3,300 x g (~6,000 RPM)**. Discard the flowthrough and reassemble the spin column with its collection tube.
19. Repeat **Step 17** one more times, for a total of two washes.
20. Spin the column, empty, for **2 minutes at 13,000 x g (~14,000 RPM)**. Discard the collection tube.
21. Transfer the spin column to a fresh 1.7 mL Elution tube. Apply 25 - 50 µL of **Elution Buffer F** to the column and let stand at room temperature for 2 minutes. Centrifuge for **1 minute at 400 x g (~2,000 RPM)**, followed by **2 minutes at 5,800 x g (~8,000 RPM)**.

➤ **Plasma/Serum DNA is ready for the downstream application of your choice.**

Table 1. Binding Buffer A, Elution Buffer C and Proteinase K to be added to different Plasma/Serum Sample Volumes

Sample Volume (mL)	Binding Buffer A (µL) (Step 1)	Elution Buffer C (µL) (Step 3)	Proteinase K (µL) (Step 4)
1.5	75	50	26
2	100	70	34
2.5	125	85	43
3	150	100	51
3.5	175	120	60
4	200	135	68
4.5	225	155	77
5	250	170	85
5.5	275	185	90
6	300	200	100

Appendix A

Cell-Free Circulating DNA Yield

Plasma/Serum Cell-free circulating DNA (cfc-DNA) is normally found in very low amounts (1 - 100 pg/μL), therefore measuring cfc-DNA concentration using common DNA quantification methods is very difficult and challenging. Typical yields of cfc-DNA vary significantly from sample to sample. Variability is also observed between samples collected from the same donor at different times during the day and therefore there is no absolute yield for cfc-DNA purified from bodily fluids including plasma or serum. Cell-free circulating DNA yield varies depending on a number of factors including age, sex, diet, exercise and most importantly the health status of the donor.

Below is a list of the most common DNA quantification methods, as well as the limit of detection for each of these methods. **Unfortunately, none of these methods can be used reliably for measuring the concentration of DNA purified from plasma or serum unless large plasma/serum volumes have been processed.** This would only be applicable if plasma/serum contains the maximum amount of DNA that can fit within the specification range of these quantification tools. It should be noted that the specifications outlined below are based on measuring a pure dsDNA, which will not be the case for the DNA purified from plasma or serum. Plasma/Serum DNA is short fragmented DNA which is usually present in less than 1000 bp. Purified plasma/serum DNA usually contains traces of proteins which will interfere with most quantification methods, leading to the overestimation of the purified DNA concentration. Therefore purified DNA contaminated with more proteins will be presented at a higher concentration as compared to DNA purified with less protein contaminants, which in this case will depend on the method used for plasma/serum DNA Isolation. ***The only reliable method that can assess the quality and the relative quantity of the purified plasma/serum DNA is qPCR amplification of a standard DNA using a small DNA amplicon such as the 5S rRNA housekeeping gene.***

Common DNA Quantification Methods

1) 2100 Bioanalyzer DNA Quantification kits

	DNA 1000 Kit	DNA 7500 Kit	DNA 12000 Kit	High Sensitivity DNA Kit
Size Range	25–1000 bp	100–7500 bp	100–12000 bp	50-7000 bp
Quantitation accuracy	20% CV*	20% CV*	25% CV*	20% CV
Quantitative range	0.5-50 ng/μL	0.5-50 ng/μL	0.5-50 ng/μL	5-500 pg/μL

2) NanoDrop 2000


- Detection Limit: 2 ng/μl (dsDNA)

3) Quant-iT™ Pico Green® dsDNA Assay Kit

- Detection Limit: 25 pg/mL

4) qPCR DNA Standard Curve

(Generated using Norgen's Low Abundance DNA Quantification Kit Cat# 57200)

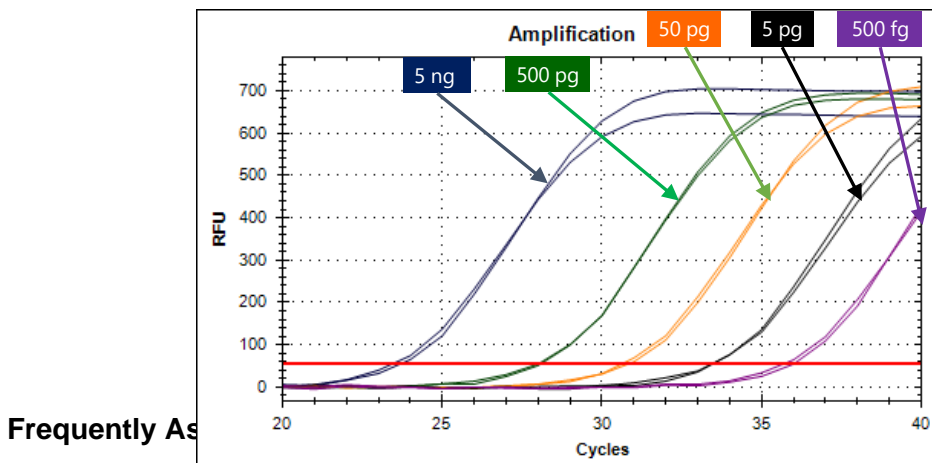

1. What if a variable speed centrifuge is not available and the speed differs from that recommended?

- A fixed speed centrifuge can be used, however reduced yields may be observed.

2. At what temperature should I centrifuge my samples?

- All centrifugation steps are performed at room temperature. Centrifugation at 4°C will not adversely affect kit performance.

3. What if I added more or less of the specified reagents' volume?

- Adding more or less than the specified volumes may reduce both the quality and the quantity of the purified DNA. Eluting your DNA in high volumes will increase the yield but will lower the concentration. Eluting in small volumes will increase the concentration but will lower the overall yield.

4. What if I forgot to do a dry spin before my final elution step?

- Your purified DNA will be contaminated with Wash Solution A. This may reduce the quality of your purified DNA and will interfere with your downstream applications.

5. Can I perform a second elution?

- Yes, but it is recommended that the 2nd elution be in a smaller volume (50% of 1st Elution). It is also recommended to perform the 2nd elution into a separate elution tube to avoid diluting the 1st elution.

6. What if my incubation time varied from what is specified in the product manual?

- Varying the incubation time will result in a reduction in your DNA yields.

7. Why do my samples show very low DNA yield?

- Plasma/Serum samples contain very little cfc-DNA. This varies from individual to individual. In order to increase the yield, the amount of Plasma/Serum input could be increased.

8. Why does my purified cfc-DNA not perform well in downstream applications?

- If a different Elution Buffer was used other than the one provided in the kit, the buffer should be checked for any components that may interfere with the application. Common components that are known to interfere are high salts (including EDTA), detergents and other denaturants. Check the compatibility of your Elution Buffer with the intended use.

9. Do I need to do an RNase treatment for my DNA Elution?

- Norgen's Plasma/Serum CFC-DNA Advanced Isolation Kit do not co-purify plasma/serum circulating RNA along with circulating DNA, therefore an RNase step is not required.

Technical Assistance

NORGEN's Technical Service Department is staffed by experienced scientists with extensive practical and theoretical expertise in sample and assay technologies and the use of NORGEN products. If you have any questions or experience any difficulties regarding Norgen's Plasma/Serum Cell-Free Circulating DNA Isolation Kits or NORGEN products in general, please do not hesitate to contact us.

NORGEN customers are a valuable source of information regarding advanced or specialized uses of our products. This information is helpful to other scientists as well as to the researchers at NORGEN. We therefore encourage you to contact us if you have any suggestions about product performance or new applications and techniques.

For technical assistance and more information, please contact our Technical Support Team between the hours of 8:30 and 5:30 (Eastern Standard Time) at (905) 227-8848 or Toll Free at 1-866-667-4362. or call one of the NORGEN local distributors (www.norgenbiotek.com) or through email at techsupport@norgenbiotek.com.

Norgen's purification technology is patented and/or patent pending. See www.norgenbiotek.com/patents

3430 Schmon Parkway, Thorold, ON Canada L2V 4Y6

Phone: (905) 227-8848

Fax: (905) 227-1061

Toll Free in North America: 1-866-667-4362